

Recorder parameters | Indicators of Digital Processing | Spectrum Estimation | Phase Scanning | Background Scanning | Auditory analysis | Conclusions

Audio recording analysis for precise determination of frequency values of stationary harmonics present in the signal in the specified range

Range from 48 to 62 Hz

Search


Analysis results:

3. 61.93 Hz


4. 61.825 Hz

Scanning accuracy: High

Signal waveform Audio for 20975 left_mono.wav , Fs=44100 Hz

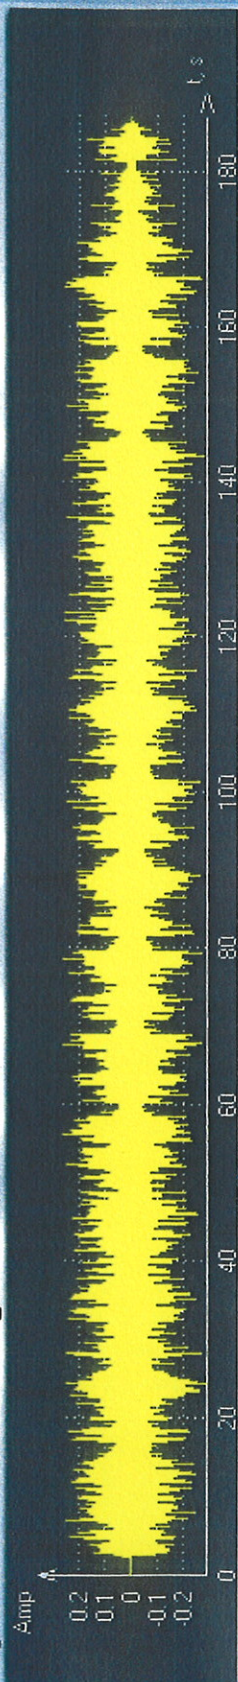

Indicator of search for a precise frequency value of stationary harmonics in the audio recording: Audio for 20975 left_mono.wav

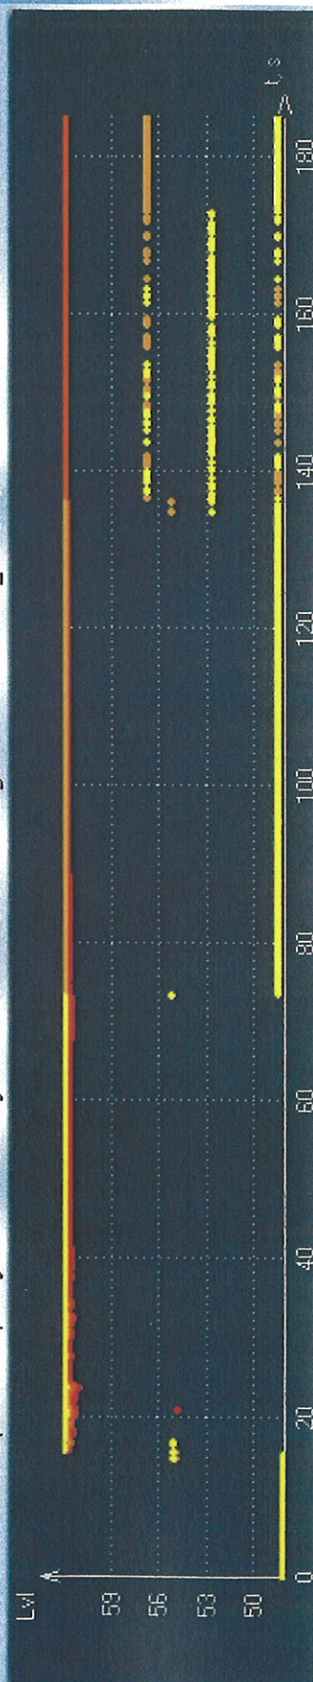

Procedure

Scanning accuracy:

Low

Normal

High

Instantaneous spectrum

